

Fig. 1

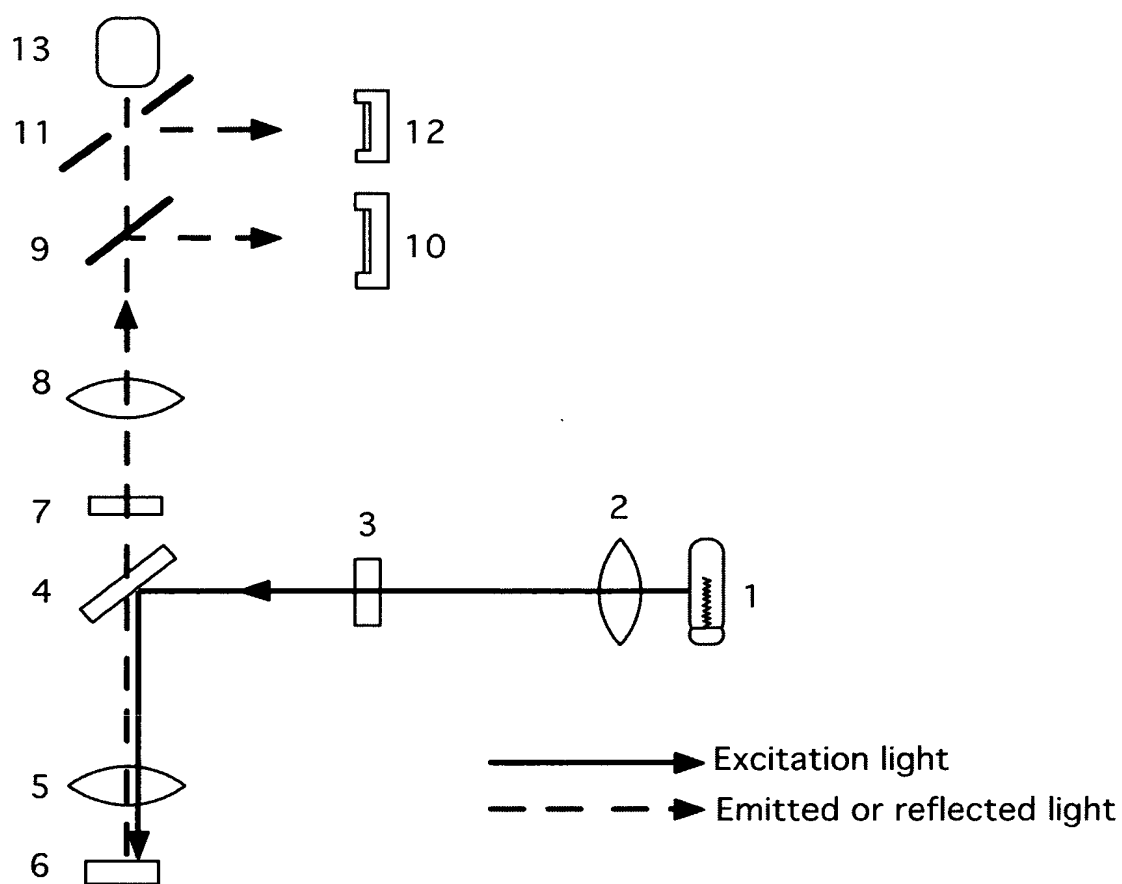


Figure 2. Schematic of microspectrometer and fluorescence detection system used to characterize the colorant dye loaded in microspheres.

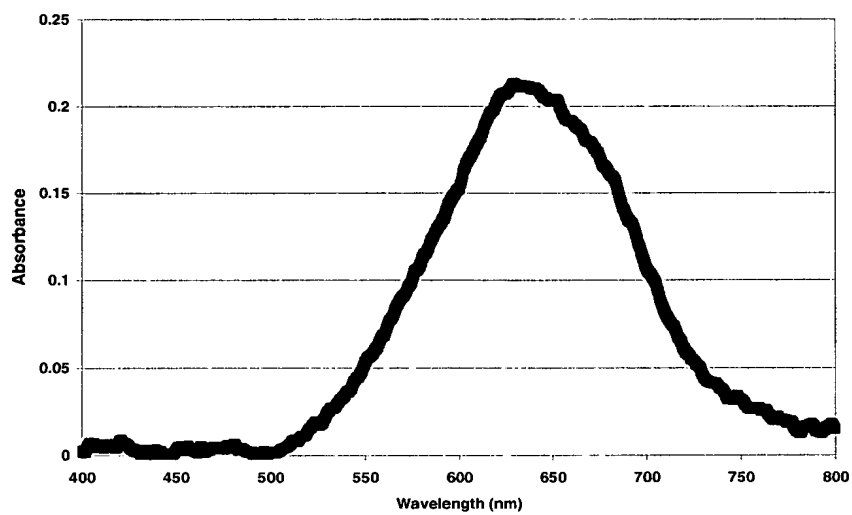


Figure 3. Spectroscopic response of CD-1 Dye loaded in microsphere.